



RC-5 USB Temperature Data Logger Operation Instruction

I. Product overview:

This data logger is mainly used for temperature recording during storage and transportation of foodstuff, medicine, chemicals and other products, especially widely used in all links of warehousing, logistics and cold chain, such as refrigerated containers, refrigerated trucks, refrigerated package, cold storage, laboratory, etc.


II. Specification:

Product size: 80mm (length) X 25mm (width) X 12 mm (height)

III. Technical parameters:




1. Temperature unit: C or F optional
2. Temperature measuring range: -30 C ~ +70 C; Resolution: 0.1 C;
3. Accuracy: ± 0.5 C (-20 C ~ +40 C); Others, +1 C;
4. Sensor: Internal NTC thermal resistor;
5. Record capacity: 32000points(MAX);
6. Record interval: 10s ~ 24hour adjustable;
7. Communication interface: USB interface;
8. Power supply: inner wide temperature CR2032 battery or power supply via USB interface;
9. Battery life: in normal temperature, if the record interval sets as 15 minutes, it could be used half a year.
10. Safe level: IP67;

IV. Initial use:

1. Install RC-5 temperature data logger data management software. Connect RC-5 with computer via USB, and install USB driver according to the Installation Tips.
2. Open RC-5 temperature data logger data management software, the data logger will automatically upload data after connected with computer. After checking the information, exit from connection interface.
3. Click the "parameters setting icon" in the tool bar. After finish the parameters setting, click "save" button to save all the parameters and exit from parameter setting interface.
4. Hold and press left button for more than 4s, the symbol  lights, then it starts recording. Click the icon of "upload data" to view the data.
5. Exit from RC-5 temperature data logger data management software.

V. Data access:

The recorded data information could be accessed from the temperature data logger. And this process will not clear the historical memory or stop record process if it is in the record status.

1. Connect the data logger with computer via USB interface, after successfully connection, the icon  shown in the LCD of data logger will light.
 2. Open RC-5 temperature data logger data management software, click the connection icon  in the tool bar. After checking the connection information, exit from connection interface.
 3. Click the data uploading icon  in the tool bar, then it will upload the data to the computer.
- Note: RC-5 parameters setting is operated through computer, for the details, please see the help file of RC-5 temperature data logger data management software.

VI. Function description:

The data logger has two button: left button and right button. Left button is to start recording and switch between menu items, and right button is to stop recording and return to the menu items.

The data logger display interfaces includes: status display, record capacity display, time display, date display, Max. temperature display, Min. temperature display, temperature upper limit display, temperature lower limit display.


If no operation within 15 minutes, the data logger will turn off the display automatically.


If the display has been turned off, short press the left button to enter the display interface. Each time short press the left button, it will shift among the display interfaces according to the sequence as described above.


Status display interface: See Figure 1







After short press the left button, it enters to the status display interface from the display turn-off status. The temperature displayed in the LCD screen is the current environmental temperature. In the status display interface:

If the symbol  lights, indicate the data logger is in the status of recording.

If the symbol  flashes, indicate the data logger is in the status of start time delay.

If the symbol  lights, indicate the data logger has stopped recording

If neither of the symbols  and  lights, indicate the data logger has not started recording.

If the symbols of  or  light, indicate the measured temperature exceeds its temperature upper/lower limit.

The temperature shown in this status display interface is the current environmental temperature.

Record capacity display interface:

When the symbol "Log" lights, it indicates that it enters to capacity display interface. The number shown in the LCD is the recorded temperature group, the interface is shown as Figure 2:



(Figure 2)

Time display interface:

In time display interface, it displays the hour and minute of the data logger. The time format is 24 hours. The display interface is as shown in Figure 3:



(Figure 3)

Date display interface:

In date display interface, it displays the month and date of the data logger, display interface is shown as Figure 4:



(Figure 4)

Note: The data below the symbol "M" indicates month, and the data below the symbol "D" indicates date.

Max. temperature display: The maximum temperature valued measured since the beginning of recording, its display interface is shown as Figure 5:



(Figure 5)

Min. temperature display: The minimum temperature measured since the beginning of recording, display interface is shown as Figure 6:




(Figure 6)

Temperature upper limit display interface shown as Figure 7:



(Figure 7)

Temperature lower limit display interface shown as Figure 8:

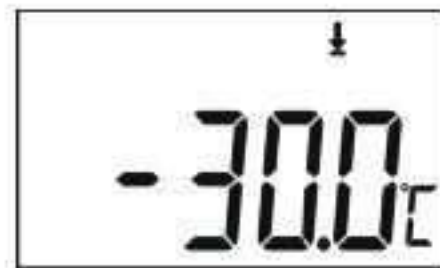

(Figure 8)

VII. Operation instruction:

1. Start recording

After setting RC-5 parameters in data management software, the function of recording has not been started yet, at this time, press the left button for more than four seconds in the status display interface, the symbol lights, and then the recording is started. If the symbol flashes, indicate the data logger is in the status of start time delay.

*** After finishing parameters setting in RC-5 temperature data logger data management software, it will clear up the recorded historical data. Please read and save data before parameter setting!**

2. Stop recording:

- ① The data logger will automatically stop recording when the recording capacity is full. In the status display interface, the symbol lights, it means recording stops.
- ② If "permit stopping by pressing button" is set, press the right button for more than four seconds, in the status display interface, the symbol lights, it means recording stops.
- ③ It could stop recording though setting in data management software. In the status display interface, the symbol lights, it means recording stops.

***After the data logger stops recording, it could not be started again by press the left button. It could only be started by setting the parameters in RC-5 data management software.**

3. Switch menu items:

By short pressing left button, display interface will switch in turn.

4. Return to the status display interface

By short pressing right button, it will return to the status display main interface from current display interface.

5. Alarm status Instruction

During recording, if the measured temperature is higher than temperature upper limit, in the status display interface, the symbol lights, indicating upper limit alarm; if the measured temperature is lower than temperature upper limit, in the status display interface, the symbol lights, indicating lower limit alarm.

6. Record interval

The record interval could be set in RC-5 data management software. After setting, it will save the data in the data logger according to the set record interval. In RC-5 data management software, when record interval is set, click the setting bar of record time length, then the software will automatically calculate the record time length.

7. Record time length

The "record time length" means the total record time when the memory reaches its full capacity.

8. Clear the recorded data

The recorded data could be cleared through setting the parameters in RC-5 data management software.

9. Inner clock and calendar

The clock could be adjusted by RC-5 data management software.

10. Sensor failure

When there is a sensor failure or over temperature range, it could query by two methods as below:

- ① When the temperature exceeds temperature range or there is a break circuit or short circuit, it will display "Err" in the position of temperature in the status display interface.
- ② There will appear an instruction of "Sensor error" in RC-5 data management software.

11. Battery level indication

The battery level could be displayed in RC-5 LCD screen.

Battery level indication	Level
	25%~100%
	10%~25%
	<10%

Note: If the battery is in a very low level (<10%), please replace the battery timely.

12. Other function:

- A. Record time delay: Set "start delay time" in the item of "parameter setting" in RC-5 data management software, then press left button for more than 4s in the status display interface, then the symbol flashes which indicate in the status of record time delay, and after started, the symbol stops flashing.
- B. Temperature unit $^{\circ}\text{C}$ or $^{\circ}\text{F}$ optional, the default setting is $^{\circ}\text{C}$

C. Serial number and user information could be set by software.

13. RC-5 temperature data logger data management software

It has the data analysis function, and could show the data in the data label or in data graph. Historical data can be queried, save, print or exported in the format of Word, Excel, TXT, or PDF. And the data management software has two versions: Windows version and Mac version. For Windows data management software, it supports the system of Windows XP, Windows 7, and Windows 8; and for Mac data management software, it supports the system of OSX10.5.6 or above. For the details, please refer to Help file of RC-5 data management software.

14. RC-5 parameter setting items in temperature data logger data management software:

Note: It is the factory default setting in the brackets. The factory default state of data logger is without starting. record interval (15 min); start delay time (0); meter station (1); Button stop (Disabled); temperature unit ($^{\circ}\text{C}$); upper temperature limit (60°C); lower temperature limit (-30°C); temperature calibration (0°C); clock set (current time); set the number (001); set user information (RC-5).

VIII. Battery replacement:



Figure 9




Figure 10



Figure 11




Figure 12




Figure 13




Figure 14




Figure 15




Figure 16

Replacement steps:

1. Rotate the battery cover counter clockwise to the position as shown in Figure 10.
 2. Remove the battery cover.
 3. Remove the old battery from the battery slot.
 4. Put the new battery into the battery slot.
 5. Place the battery cover in the position shown in Figure 14.
 6. Rotate the battery cover clockwise from Position shown in Figure 15 to the position shown in Figure 16.
- Note: The pole piece in the bottom of the battery slot is negative.

IX. Accessory list

Standard accessory list
 One RC-5 temperature data logger
 One operation instruction

Note: The software or user manual could also be downloaded in our website: www.e-elitech.com

Optional accessory list

One software installation CD